

Newman  Medical

Employee Owned & Operated

simple ABI ™

with CUFF:LINK™

Vascular Diagnostic System

User Manual



Newman Medical
5350 Vivian Street, Unit C
Arvada, CO 80002
1-800-267-5549
info@newman-medical.com
www.newman-medical.com

COMMON TERMINOLOGY

ABI	Ankle Brachial Index - the ratio of the ankle systolic blood pressure divided by the brachial (arm) systolic blood pressure.
Distal	Points situated away from the center of the body – i.e. “downstream”. An example - the ankle is distal to the calf.
Distal Pressure	A pressure taken distal to the method of occlusion. I.e. taking the brachial pressure below (distal to) the cuff.
DP (or DPA)	Dorsalis Pedis Artery --- the artery on top of the foot. Used in the ABI exam.
MHz	Megahertz – Millions of cycles per second --the frequency of the sound transmitted by a vascular probe is measured in megahertz - 8 million cycles per second, for example.
PAD	Peripheral Artery Disease – Typically atherosclerosis (also known as hardening of the arteries) in the leg.
PPG	Photoplethysmography –detects the pulse using reflected light from a small emitter/detector combination.
Proximal	Points situated nearer to the center of the body – i.e. “upstream”. An example – the calf is proximal to the ankle.
PT – (or PTA)	Posterior Tibial Artery – artery on the inside of the ankle used in the ABI exam.
PVD	Peripheral Vascular Disease – Includes venous as well as arterial disease.
PVR	Pulse Volume Recording – a means of evaluating the condition of the arteries by looking at a waveform of small changes in cuff pressure caused by pulses in the arteries under the cuff.
Reactive Hyperemia	The transient increase in organ blood flow that occurs following a brief period of restriction of blood flow. In lower arterial this is typically done by placing a cuff on the thigh and occluding blood flow for 3-5 minutes, then quickly releasing. An extremely painful exam.
Segmental	Pressures and PVRs just like the ABI but done in more cuffs on the leg to assist in localizing the site of any occlusion. The Doppler probe can remain at the ankle for the pressures.
TBI	Toe Brachial Index – the ratio of the pressure in the toe divided by the brachial pressure. It is generally measured with a small toe cuff and a PPG probe

Contents

Chapter 1 – About simpleABI	2
Chapter 2 – Safety	2
Safety of Equipment	2
Intended Use	2
Indications	2
Contraindications.....	3
Chapter 3 – Setting up your simpleABI	5
Chapter 4 – simpleABI Reporting Software.....	6
Chapter 5 – Performing Exams.....	8
Interpretation of waveforms	8
ABI-Q Examination.....	9
ABI Examination.....	10
The ABI with Toe (TBI) Examination	12
Segmental Examinations	14
ABI with Exercise Examination.....	17
The ABI Stress Examination	18
Chapter 6 – Detailed Description.....	20
Chapter 7 – Tips & Troubleshooting	20
Chapter 8 – Maintenance, Cleaning & Disposal	21
Chapter 9 – Specifications.....	21
Chapter 10 – Electromagnetic Compatibility.....	24
Chapter 11 – Warranty, Service, & Support	26

Chapter 1 – About simpleABI

Congratulations on your purchase of a simpleABI Cuff-Link™ System from Newman Medical.

The simpleABI Cuff-Link™ was designed to be the easiest and most intuitive system on the market for initial vascular assessment. We hope you find that to be the case. If not, please do not hesitate to call us and let us know how we can improve the product for you.

What is included with simpleABI Cuff-Link Systems

- Cuff-Link Control Unit – provides control and connection of vascular cuffs , Doppler, PPG and computer in the patient environment
- Cuff-Link Remote Control
- Doppler Probes(s)
- PPG Probe
- Vascular Cuffs
- USB Cable
- Laptop PC - simpleABI is designed to work with a computer certified to IEC 60601-1, IEC-62368-1 or IEC 60950-1 and running Windows 10 (32 or 64 bit) or Windows 11 (64 bit) in the Operator environment.
- simpleABI User Manual

Chapter 2 – Safety

Safety of Equipment

simpleABI Systems are medical equipment. Although designed to withstand everyday use, care must be taken to ensure safe and continued operation. Do not abuse equipment. simpleABI Systems were designed according to domestic and International consensus safety standards. Throughout design of this product, safety was the paramount concern. In view of that, this product was designed according to the principle of reducing risk AFAP (**As Far As Possible**).

Intended Use

This product is intended for use by health care providers for detection of blood flow in the veins and arteries and as an aid in the diagnosis of peripheral arterial disease.

CAUTION: Federal law restricts this device to sale by or on the order of a physician or other licensed practitioner.

Indications

Indications for noninvasive physiologic testing

Common indications for lower extremity arterial physiologic evaluation include, but are not limited to:

- Peripheral arterial disease (PAD)
- Exercise-related limb pain (claudication symptoms)
- Limb pain at rest
- Extremity ulcer/gangrene
- Assessment of healing potential
- Absent peripheral pulses
- Digital cyanosis
- Cold sensitivity

- Arterial trauma and aneurysms
- Suspected arterial embolization
- Pre-procedure assessment (e.g., angioplasty, stent, bypass graft)
- Follow-up endovascular procedure (e.g., angioplasty, stent)
- Follow-up bypass graft
- Prognosis for healing (e.g., ulcerations, amputations)

Indications for exercise and/or treadmill testing

- Normal resting lower extremity arterial segmental limb pressures and pulse volume recordings at rest, in the context of a history of intermittent claudication
- Resting lower extremity segmental limb pressures and pulse volume recording amplitudes mildly abnormal at rest (i.e. ABI > 0.80 but < 0.96) in a patient with a history of intermittent claudication

Contraindications

Contraindications for noninvasive physiologic testing

Contraindications for lower extremity arterial physiologic evaluation include, but are not limited to:

- Morbidly obese patients in whom a high-thigh pressure may be not obtainable
- Casts, dressings, staples and/or open wounds
- Suspected or known acute deep venous thrombosis (DVT)
- Incompressible vessels with arterial calcification (TBI may be obtained)
- Post-interventional procedure (e.g., stenting, bypass graft)
- Recent surgery, trauma, ulcers, casts or dressings that should not be compressed by a blood pressure cuff
- Involuntary movement/tremors may render waveform collection suboptimal or unreliable

Contraindications for exercise and/or treadmill testing

Contraindications of exercise and/or treadmill testing the lower extremities include, but are not limited to:

- Rest pain
- Noncompressible vessels on a resting study
- Acute deep venous thrombosis
- Shortness of breath at rest or with minimal exertion
- Uncontrolled angina, or a physical disability that limits patient's ability to ambulate on a treadmill.

Contraindications of blood pressure measurements

Contraindications of blood pressure measurements include, but are not limited to:

- Do not take an arm pressure in an arm with a shunt or dialysis graft.
- Patients with a side affected by stroke, mastectomy or renal fistula should avoid having blood pressure readings taken on this side.
- If a patient has an IV catheter in one arm, use the other arm to take the reading to prevent potential damage to the catheter and interruption of administration of medication.
- Lymphedema
- Paresis or paralysis
- Arterial or venous lines

WARNING: The device is not to be used on or near the eyes.

WARNING: The device is for use only on intact skin.

WARNING: Do not leave a cuff inflated at high pressures for an extended period of time when on a patient.

WARNING: Probes are not intended to be used on open skin. If there is evidence of open wound contamination, disinfect the probe before using again as described Chapter 8 – Maintenance and Cleaning.

WARNING: Any open lesion with the potential for contamination should be covered with an impermeable dressing.

WARNING: Connect only to a computer certified to IEC/AAMI 60601-1, IEC/UL 62368-1 or IEC/UL 60950-1. Computer is not intended for patient contact.

WARNING: To avoid safety or compliance issues, no modification of this equipment is allowed.

WARNING: Components of simpleABI Systems are not user serviceable. To maintain patient safety, do not maintain or clean equipment while in use.

WARNING: Not intended for use in conjunction with HF Surgical equipment.

WARNING: Doppler probe is not intended for immersion in liquids.

CAUTION: The device is not to be plugged into a telephone or modem system.

CAUTION: Do not inflate a cuff when it is not on a patient.

AIUM Statements

As Low As Reasonably Achievable (ALARA) Principle

Approved May 19, 2020

The potential benefits and risks of each examination should be considered. The as low as reasonably achievable (ALARA) principle should be observed when adjusting controls that affect the acoustic output and by considering both the transducer dwell time and overall scanning time. Practicing ALARA requires that users do all of the following:

1. Apply correct examination presets if built into the diagnostic ultrasound device. The review of manufacturer default presets for appropriateness is encouraged.
2. Adjust the power to the lowest available setting that provides diagnostic-quality images. If appropriate, reduce power at the end of each examination so the next user will start with the lowest acoustic output setting.
3. Monitor the mechanical index (MI) and thermal index (TI). Know the recommended upper limit of the MI, TI, and related duration limitations for the type of examination being performed.
4. Move/lift the transducer when stationary imaging is not necessary to reduce the dwell time on a particular anatomic structure. When possible, avoid fields of view that include sensitive tissues such as the eye, gas-filled tissues (lung and intestines), and fetal calcified structures (skull and spine)
5. Minimize the overall scanning time to that needed to obtain the required diagnostic information.

Prudent Use and Clinical Safety

Approved May 20, 2019

Diagnostic ultrasound has been in use since the late 1950s. Given its known benefits and recognized efficacy for medical diagnosis, including use during human pregnancy, the American Institute of Ultrasound in Medicine herein addresses the clinical safety of such use: No independently confirmed adverse effects caused by exposure from present diagnostic ultrasound instruments have been reported in human patients in the absence of contrast agents. Biological effects (such as localized pulmonary bleeding) have been reported in experimental mammalian systems at diagnostically relevant exposures, but the clinical relevance of such effects is either not significant or is not yet known. Increased outputs and time of exposure can increase the likelihood of bioeffects. Ultrasound should be used only by qualified health professionals to provide medical benefit to the patient. Ultrasound exposures during examinations should be as low as reasonably achievable (ALARA)

Safety in Research Using Diagnostic Ultrasound

Approved May 20, 2019

Diagnostic ultrasound has been in use since the late 1950s. There are no confirmed adverse biological effects on patients resulting from this use. Although no hazard has been identified that would preclude the prudent and

conservative use of diagnostic ultrasound in research, experience from normal diagnostic practice may not be relevant to potential extended exposure times and altered exposure conditions in research. It is therefore considered appropriate to make the following recommendation: When examinations are carried out for purposes of research, ultrasound exposures should be as low as reasonably achievable (ALARA) within the goals of the study. In addition, informed consent, using a form approved by an Institutional Review board, should be obtained from the patient. Informed consent forms should include information about the anticipated exposure conditions and how these compare with normal diagnostic practice. Repetitive and prolonged exposures on a single patient should be justified and consistent with prudent and conservative use.

Chapter 3 – Setting up your simpleABI


Installation of your simpleABI is straightforward but may require a few common tools. This installation is typically handled by a trained Newman Medical salesperson.

Stand Assembly

If a stand was included with the order, please see the assembly instructions supplied with the stand.

1. Place computer onto mounting plate, ensuring all loop tabs on PC line up with respective hook tabs on mounting plate.
 - a. It is helpful to first check how the computer aligns on the mounting plate prior to placing hook and loop tabs.
2. Place all cuffs into basket.
3. Connect the Cuff-Link control unit to the computer with the included USB cable. Insert the Cuff-Link Remote cable firmly into the control unit. Attach the hoses to the Cuff-Link control unit as shown below. Hoses are color coded to aid attachment. Depending on model chosen, systems will have 4 or 8 tubes. Both units are shown below.

NOTE: Care should be taken when attaching hoses. Do not overtighten connectors or damage may occur.

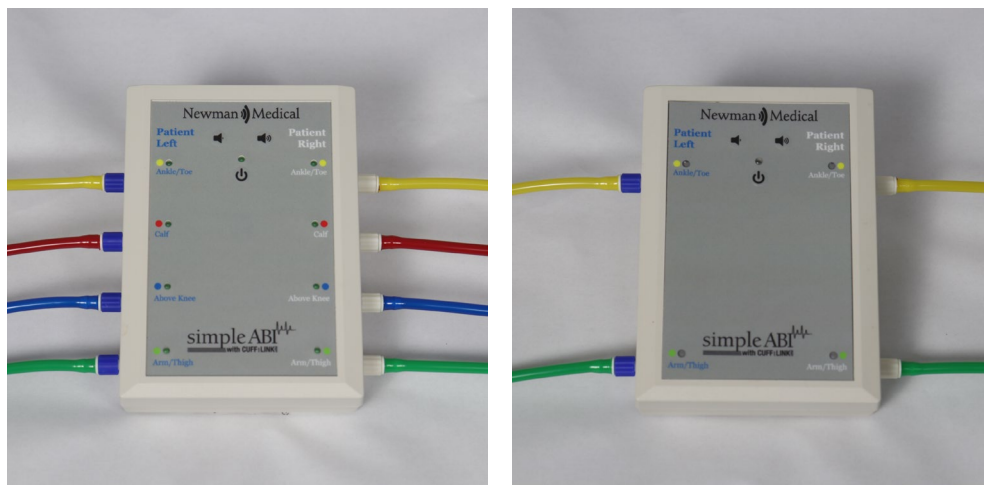

4. Attach Doppler probe and PPG probe to Cuff-Link Control Unit.

FIELD INSTALLATION OF SIMPLEABI SOFTWARE

This section applies only to systems where the software is installed in the field – computers shipped from Newman Medical already have the software loaded and this section does not apply.

CAUTION: simpleABI is only supported on the following Windows Operating Systems:

- Windows 10 (32 or 64 bit)
- Windows 11 (64 bit)

Do not install on any other operating systems prior to contacting Newman Medical Technical Support for information.

CAUTION: Use of other applications (word processing, games, internet) is not an appropriate use of a medical device and must be avoided to ensure proper operation of the simpleABI system.

Software Installation Directions

1. Plug in included USB Flash Drive into PC
2. Copy *.msi to C:\ (*.msi file will have different names depending on simpleABI system purchased)
3. Double Click *.msi file to begin installation

NOTE: ***DO NOT INSTALL OFF REMOVABLE MEDIA***

Cuff-Link Driver Installation

1. Plug in Cuff-Link control unit and make sure to power on the unit. Cuff-Link uses standard Windows drivers and is 'plug and play'.
2. Driver should be properly installed and can be checked by opening simpleABI Reporting Software.
 - a. If installed properly, top of window will display 'Connected' and the following icon.



- b. If not installed properly, top of window will display 'Not Connected' and the following icon.



Chapter 4 – simpleABI Reporting Software

File Menu

Beginning a new exam

From the computer Desktop, select the simpleABI icon. The simpleABI start-up screen with menu items on the top will appear. Select *File* → *New* and the exam to be performed. Depending on the system chosen, you will have different choices of exams. Choose an exam and it will open on the screen..

Loading an Exam

From the simpleABI start-up screen, Select *File* → *Load* and the exam to be performed. You may select any previously report to populate the loading exam with data relevant to the exam. I.e. you can load an ABI exam into a segmental exam; all patient information and arm/ankle pressures and waveforms from previous exam will be loaded. You would need only to perform upper leg pressure/waveform measurements. Depending on the system chosen, you will have different choices of exams. Choose an exam to load, select a previous exam and it will open on the screen.

Saving an Exam

You can save your finished report using CTRL+S or selecting *File* → *Save*. Files are appended with Patient ID and a timestamp to differentiate exams. You may also overwrite this default file name. By default, the save command automatically saves the exam in PDF and XML data files. You may select additional file types under *Edit* → *Output Formats* (TIFF, BMP, JPG, CSV)

Printing an Exam

You can print your exams using CTRL+P or selecting *File →Print*

Closing an exam

You can close any open exam or editing form by selecting *File →Close Form* or CTRL+W

Exiting the software to exit software, select *File →Close Form* or ALT+F4.

Edit Menu

REPORT INFORMATION You can edit referring doctor, examiner, interpreting doctor, and practice information and logo under this menu item. Logos and signatures must be of BMP format to be loaded into the system. There are some samples pre-filled and you can add, edit, or delete these as you deem necessary.

Add/Delete/Edit Doctor/Examiner/Practice Information/Logos

Under the *Edit* menu there are multiple options for editing the configuration of your software. You may add, delete, and edit practice information, examiner information, doctor information, output formats, impressions, and ICD codes. You can also upload practice logos to customize reports.

To close any editing form, select *File →Close Form*

OUTPUT FORMATS You can select from different formats to fit your needs. Options available are PDF, JPG, BMP, TIF, CSV (XML is our data format and cannot be deselected). By default, PDF is selected.

IMPRESSIONS exam impressions can be pre-filled using this menu item. Use only numbers for impression numbers.

ICD CODES ICD codes can be edited, added or deleted using this menu item. There are many pre-populated ICD codes; however, only some relevant codes have been selected to 'Show in List' on exams. You may choose to edit these as you deem necessary.

CHART OPTIONS chart options allow different scaling or auto-scale for PVR waveforms. By default, a scaling factor of 1.00 is selected.

DICOM SETUP (OPTIONAL) An optional license key must be purchased to access DICOM setup options. simpleABI DICOM provides the ability to connect to a PACS server, query worklist, and send image or Standard reporting DICOM formats.


Help

Help is found by selecting the Help Menu. You may view system information as well as, with an internet connection, be directed to Newman Medical's home page where you can browse to our support pages with helpful hints and videos on using your simpleABI System.


Chapter 5 – Performing Exams

Interpretation of waveforms


Pulse Volume Recording (PVR) is used to measure the change in pressure in the cuff caused by the small changes in volume that occur with each pulse. The analysis of the waveform is based on the shape of the waveform rather than the amplitude. PVRs are not affected by calcified arterial walls and are relatively easy to perform.

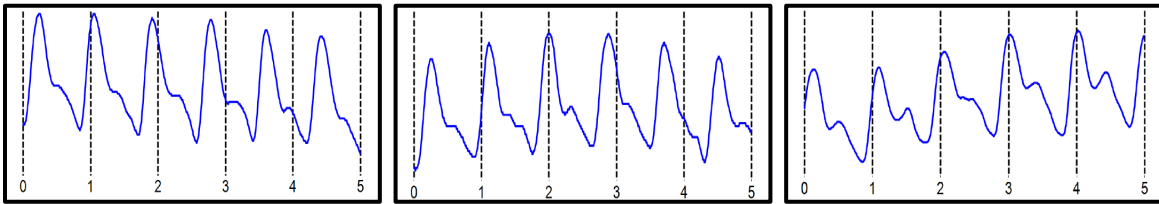

Normal: Waveforms with a rapid rise and a prominent reflected wave (dicrotic notch)

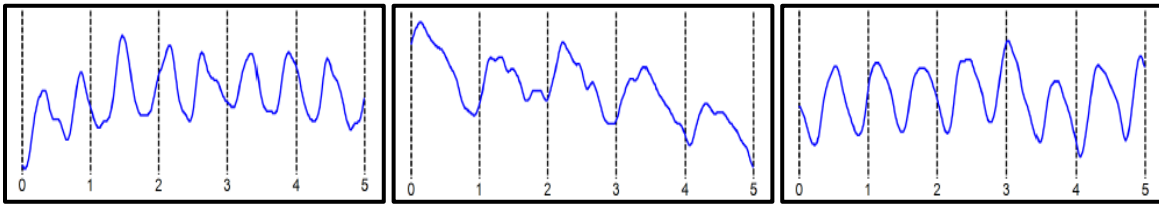

Moderately Abnormal: Waveform starts to broaden and no reflected wave.

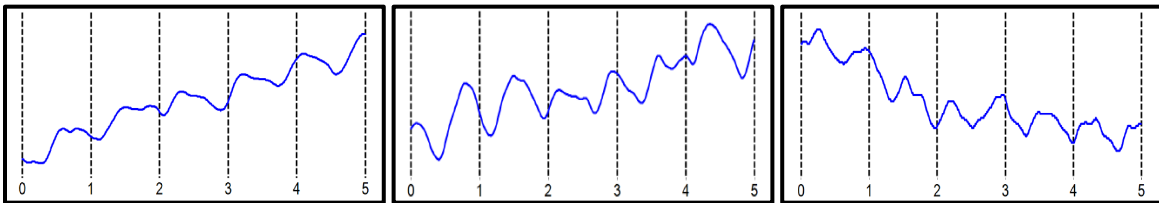

Abnormal: No reflected wave, slow rise. Potential 'flatline'

Determining site of occlusion with PVR waveforms:¹ A normal waveform at a site indicates that there is likely not occlusive disease proximal to that cuff.

¹ Daigle, Robert J., Techniques in Noninvasive Vascular Diagnosis, Summer Publishing, www.summerpublishing.com

ABI-Q Examination

Purpose & Background

The ABI-Q™ procedure is a 1-2 minute exam to quickly and effectively assess the lower extremity arteries for peripheral artery disease. It utilizes PVR waveforms at both ankles.


The ABI-Q™ exam is a diagnostic test that examines arterial waveforms to determine the need for further vascular evaluation.

Opening the exam

On the computer desktop, double click the simpleABI icon. When the program opens select *File* → *New* → *New ABI-Q Report*. The report will open and you can enter patient information, risk factors, symptoms, ICD codes, etc.

Attaching cuffs

Have the patient lie down in the supine position relaxed, head and heels supported in a comfortably warm room. Wrap appropriately sized cuffs (usually 10cm on the ankles). On the legs, have the patient place their feet flat on the table with knees bent as you apply the cuff above their ankle. Cuffs should fit snugly so that fingers should slide between the cuff and limb with difficulty. The lower edge of the ankle cuff should be about an inch above the top of the medial malleolus (ankle bone).

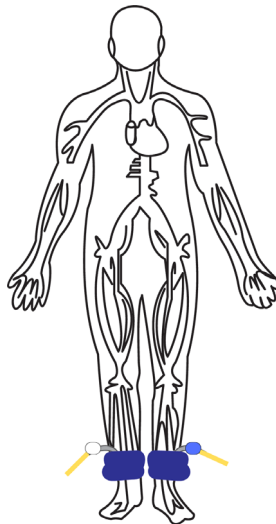

Obtaining Waveforms

1. To obtain a **PVR waveform** click on the right box for taking a waveform in the middle of the screen. Press the button with the **waveform** image on it on the top right of the remote. The cuff will inflate to 80 mmHg pressure, slowly deflate to 65 mm and then hold that while the waveform is obtained. The patient should remain still during the measurement; the waveform will start to appear after the cuff reaches 65 mm.
2. If you are not satisfied with the waveform, just push the **waveform** button again
3. Press either **Next** after the waveform is obtained to move to the other side.

Left Side

1. Repeat steps above for the left side.

Saving/Printing

Save the report by selecting *File* → *Save* or pressing CTRL+S. Print the report by selecting *File* → *Print* or pressing CTRL+P.

Exam Helpful Hints

How Pulse Volume Recording (PVR) Works

- Blood volume in the legs increases with each pulse and this increases the pressure in the cuff. These small changes are recorded and saved as the PVR waveform

Advantages of PVR

- PVRs provide a measure of the total blood flow through the limb unlike Doppler waveforms which show only the flow in the artery directly in front of the probe.
- PVRs are not affected by calcified arteries (if the ABI is greater than 1.4 it is likely due to calcified arteries)
- PVRs are easier to perform than Doppler waveform analysis
- The only skill required to acquire PVRs is the ability to wrap vascular cuffs snugly
- PVRs require patient cooperation; limb motion affects the waveform. Patients should be instructed not to move or talk during this test

ABI Examination

Purpose & Background


The ABI has become the best known and standardized test for PAD. Fundamentally it is the systolic blood pressure taken with the cuff at the ankle divided by the systolic pressure taken with the cuff on the upper arm.

Opening the Exam

On the computer desktop, double click the simpleABI icon. When the program opens select *File* → *New* → *New ABI Report*. The report will open and you can enter patient information, risk factors, symptoms, ICD codes, etc.

Attaching cuffs

Wrap appropriate cuffs at each site. Attach the hoses from the Cuff-Link Control Unit to cuffs as shown below. The green connectors go to the arm cuffs and yellow to the ankles. White hoses go to the patient's right side, blue to the left. *NOTE* the image is reversed as if you are looking at the patient lying down.

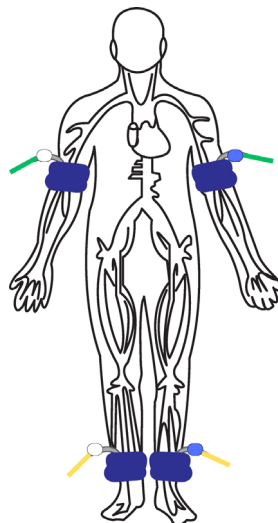

Arm Pressure

1. Begin with the right brachial. Place the Doppler probe at a 45-degree angle to the skin over the radial or brachial artery. Use plenty of gel and slowly move the probe laterally until the best signal is obtained.
2. Press and hold **Inflate** on the Cuff-Link Remote (shown above) and inflate the cuff until you no longer hear the signal - continue for an additional 10-20 mmHg.
3. Release **Inflate** and the cuff will automatically deflate at the suggested rate of 2mmHg/second.
4. When you hear the Doppler signal return, pressing **Pressure** will store the pressure value in the exam.



Ankle Pressures

1. Press **Next** on the remote and the system will move to the Dorsalis Pedis (DP) site. Find the arterial signal using the Doppler probe on the dorsalis pedis artery on top of the foot. Obtain the arterial pressure in the same manner you did on the arm. (Hold **Inflate** until occlusion, release **Inflate**, press **Pressure** on Doppler signal return)



2. Press **Next** and the system will move to the posterior tibial (PT) site. Find the Doppler signal on the posterior tibial artery. Obtain the arterial pressure. (Hold **Inflate** until occlusion, release **Inflate**, press **Pressure** on Doppler signal return).



Waveform

1. Press **Next** and the system will move to the waveform site. Press and release the button with the **Waveform** image on the top right of the remote. The cuff will inflate to 80 mmHg pressure, slowly deflate to 65 mm and then hold that while the waveform is obtained. The waveform will start to appear when the cuff has reached 65mmHg. The patient should remain as still as possible during the measurement.

Left Side

2. Repeat steps above for the left side.

The interpretation of the ABI values is based on recent guidelines.²

Saving/Printing

Save the report by selecting *File* → *Save* or pressing CTRL+S. Print the report by selecting *File* → *Print* or pressing CTRL+P.

Exam Helpful Hints

If the ankle pressure is high, above 200 mmHg, or the cuff cannot obliterate the Doppler sounds, this indicates that the artery may be incompressible due to calcification.

The ABI with Toe (TBI) Examination

Purpose & Background

The ABI with Toe exam is typically performed after an ABI has been done, especially if the larger ankle arteries appear to be incompressible (pressure over 200mmHg) or anytime more information is needed about small vessel disease. The TBI is done using the PPG probe. The patient is supine and rested in a warm room.

Opening the exam


On the computer desktop, double click the simpleABI icon. When the program opens select *File* → *New* → *New ABI with Toe Report*. The report will open and you can enter patient information, risk factors, symptoms, ICD codes, etc.

² 2016 AHA/ACC Guideline on the Management of Patients With Lower Extremity Peripheral Artery Disease, J Am Coll Cardiol. 2017 Mar, 69 (11) e71-e126.

Attaching cuffs

Wrap appropriate cuffs at each site. Attach the hoses from the Cuff-Link control unit to cuffs as shown below. The green connectors go to the arm cuffs and yellow to the ankles or toes. White hoses go to the patient's right side, blue to the left.

If you have performed a previous ABI Exam, you may load the results into this exam by selecting *File* → *Load* → *ABI with Toe Report* and selecting the ABI Exam you previously performed.

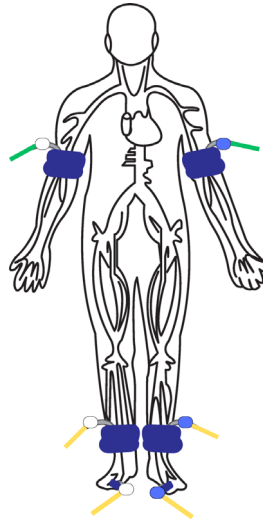

Brachial Pressure

1. Begin with the right brachial. Place the Doppler probe at a 45-degree angle to the skin over the radial or brachial artery. Use plenty of gel and slowly move the probe laterally until the best signal is obtained.

2. Press and hold **Inflate** on the Cuff-Link Remote (shown above) and inflate the cuff until you no longer hear the signal - continue for an additional 10-20 mmHg.
3. Release **Inflate** and the cuff will automatically deflate at the suggested rate of 2mmHg/second.
4. When you hear the Doppler signal return, pressing **Pressure** will store the pressure value in the exam.

Ankle Pressures

1. Press **Next** on the remote and the system will move to the Dorsalis Pedis (DP) site. Find the arterial signal using the Doppler probe on the dorsalis pedis artery on top of the foot. Obtain the arterial pressure in the same manner you did on the arm. (Hold **Inflate** until occlusion, release **Inflate**, press **Pressure** upon Doppler signal return)
2. Press **Next** and the system will move to the posterior tibial (PT) site. Find the Doppler signal on the posterior tibial artery. Obtain the arterial pressure. (Hold **Inflate** until occlusion, release **Inflate**, press **Pressure** upon Doppler signal return)

Ankle Waveform

1. Press **Next** and the system will move to the waveform site. Press and release the button with the **Waveform** image on the top right of the remote. The cuff will inflate to 80 mmHg pressure, slowly deflate to 65 mm and then hold that while the waveform is obtained. The waveform will start to appear when the cuff has reached 65mmHg. The patient should remain as still as possible during the measurement.

Toe Pressure

1. Press **Next** on the remote and the system will move to the Toe pressure field. Place the PPG sensor on the fleshy part of the toe opposite the toenail. Use cohesive tape or double sided tape to attach PPG sensor to the toe. Wait for consistent pulsatile waveform to appear. A warm towel aids blood flow in the toes. Obtain the toe pressure by inflating the cuff until the PPG waveform 'flatlines' and release **Inflate**. When pulsatile waveform reappears, press **Pressure** to store the pressure value in the exam. ***Note*** The toe cuff inflates rapidly – light taps of the **Inflate** button are best.

Toe Waveform

1. Press **Next** and the system will move to the waveform site. Press and release the button with the **Waveform** button on the top right of the remote. The PPG waveform will begin to scroll in the waveform field. When you are satisfied with the waveform press either the **Next** or the **Waveform** button to store the PPG waveform. Patient should remain as still as possible during the measurement.

Left Side

1. Repeat the above pressures and waveform sequence for the left side of the patient.

Saving/Printing

Save the report by selecting *File* → *Save* or pressing CTRL+S. Print the report by selecting *File* → *Print* or pressing CTRL+P.

Exam Helpful Hints

A warm toe is a big help. Keep the toe covered if you can with a towel or warm towel, if available. Let the patient rest and relax before inflating the cuffs. Anchor the cord from the PPG sensor to the foot with some adhesive tape.

Toe pressures are difficult to obtain in patients with small vessel disease. Pressures can be obtained with the Doppler probe as well, but it is more difficult as the digit arterial signal is hard to locate.

Segmental Examinations

Purpose & Background

A segmental exam of the leg is an extension of the ABI exam. In this test, you can attempt to localize the site of an occlusion by taking the pressures and waveforms at more locations on the leg.

By observing the difference in pressure between adjacent sites on the leg you can tell if there is an occlusion between those sites.


A greater than 20mmHg difference between sites is considered positive for a significant stenosis in the artery between or under the cuff.

Opening the exam

On the computer desktop, double click the simpleABI icon. When the program opens select *File* → *New* → *3 cuff Segmental Report (or 4 cuff)*. The report will open and you can enter patient information, risk factors, symptoms, ICD codes, etc.

Attaching cuffs

Wrap appropriate cuffs at each site. Attach the hoses from the Cuff-Link control unit to cuffs as shown below. The green connectors go to the arm (or thigh) cuffs, red to the calves, blue to above the knee cuffs, and yellow to the ankles. White hoses go to the patient's right side, blue to the left. *NOTE* the image is reversed as if you are looking at the patient lying down

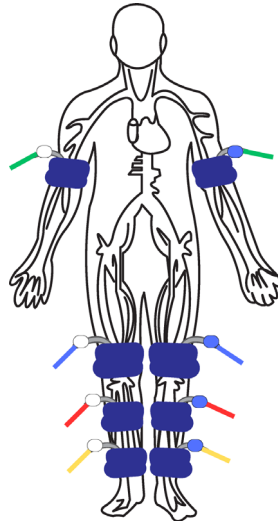

Brachial Pressure

1. Begin with the right brachial. Place the Doppler probe at a 45 degree angle to the skin over the radial or brachial artery. Use plenty of gel and slowly move the probe laterally until the best signal is obtained.
2. Press and hold **Inflate** on the Cuff-Link Remote (shown above) and inflate the cuff until you no longer hear the signal - continue for an additional 10-20 mmHg.
3. Release **Inflate** and the cuff will automatically deflate at the suggested rate of 2mmHg/second.
4. When you hear the Doppler signal return, pressing **Pressure** will store the pressure value in the exam.

Ankle Pressures

1. Press **Next** on the remote and the system will move to the Dorsalis Pedis (DP) site. Find the arterial signal using the Doppler probe on the dorsalis pedis artery on top of the foot. Obtain the arterial pressure in the same manner you did on the arm. (Hold **Inflate** until occlusion, release **Inflate**, press **Pressure** on Doppler signal return)
2. Press **Next** and the system will move to the posterior tibial (PT) site. Find the Doppler signal on the posterior tibial artery. Obtain the arterial pressure. (Hold **Inflate** until occlusion, release **Inflate**, press **Pressure** on Doppler signal return)

Ankle Waveform

Press **Next** and the system will move to the waveform site. Press and release the button with the **Waveform** image on the top right of the remote. The cuff will inflate to 80 mmHg pressure, slowly deflate to 65 mm and then hold that while the waveform is obtained. The waveform will start to appear when the cuff has reached 65mmHg. The patient should remain as still as possible during the measurement.

Calf Pressure & Waveform

1. Press **Next** on the remote and the system will move to the calf site. Obtain the arterial pressure and waveform in the same manner you did on the ankles.

Above Knee Pressure & Waveform

1. Press **Next** on the remote and the system will move to the above knee site. Obtain the arterial pressure and waveform in the same manner you did on the ankles.

Thigh Pressure & Waveform (Certain segmental exams)

1. Press **Next** on the remote and the system will move to the thigh site. Obtain the arterial pressure and waveform in the same manner you did on the ankles.

Left Side

Repeat the above pressures and waveform sequence for the left side of the patient

Toe Pressure (Certain segmental exams)

1. Press **Next** on the remote and the system will move to the Toe pressure field. Place the PPG sensor on the fleshy part of the toe opposite the toenail. Use cohesive tape or double sided tape to attach PPG sensor to the toe. Wait for consistent pulsatile waveform to appear. A warm towel aids blood flow in the toes. Obtain the toe pressure by inflating the cuff until the PPG waveform 'flatlines' and release **Inflate**. When pulsatile waveform reappears, press **Pressure** to store the pressure value in the exam. ***Note*** The toe cuff inflates rapidly – light taps of the **Inflate** button are best.

Toe Waveform (Certain segmental exams)

1. Press **Next** and the system will move to the waveform site. Press and release the button with the **Waveform** button on the top right of the remote. The PPG waveform will begin to scroll in the waveform field. When you are satisfied with the waveform press either the **Next** or the **Waveform** button to store the PPG waveform. Patient should remain as still as possible during the measurement.

Saving/Printing

Save the report by selecting *File* → *Save* or pressing CTRL+S. Print the report by selecting *File* → *Print* or pressing CTRL+P.

Exam Helpful Hints

Elevated Leg Pressures

If the ankle pressure is high, above 200 mmHg, or the cuff cannot obliterate the Doppler sounds, this indicates that the artery may be incompressible due to calcification.

Efficient, less painful protocols

Current CPT guidelines for CPT code 93923 state that if PVR waveforms are being utilized, only pressures at the ankles must be obtained. **Pressures** do not need to be obtained at the calf, above knee, or thigh.

This has many advantages – most notable

1. This protocol significantly reduces the time necessary for this exam.
2. This protocol will be significantly less painful for your patients

ABI with Exercise Examination

Purpose & Background

The ABI with Exercise test is useful for differentiating true vascular claudication from other non-vascular pains. The stress can be produced by treadmill walking exercise (CPT 93924) or by toe/heel raises (CPT 93923).


Contraindications

- Questionable cardiac status
- Severe pulmonary disease
- Ischemic rest pain, ulceration, or ankle pressures <40mm Hg
- Non-compressible tibial arteries
- Do not perform the ABI exam on someone suspected of having acute deep venous thrombosis, and do not take an arm pressure in an arm with a shunt or dialysis graft.

Explain to the patient that they will be exercising, either walking or doing toe raises, or until pain stops them. Ask them to tell you when and where pain occurs. Remind them to report any chest pain, shortness of breath, or severe fatigue.

Opening the exam On the computer desktop, double click the simpleABI icon. When the program opens select *File → New → New ABI with Exercise Report*. The report will open and you can enter patient information, risk factors, symptoms, ICD codes, etc.

Attaching cuffs Wrap appropriate cuffs at each site. Attach the hoses from the Cuff-Link control unit to cuffs as shown below. The green connectors go to the arm cuffs and yellow to the ankles. White hoses go to the patient's right side, blue to the left. *NOTE* the image is reversed as if you are looking at the patient lying down

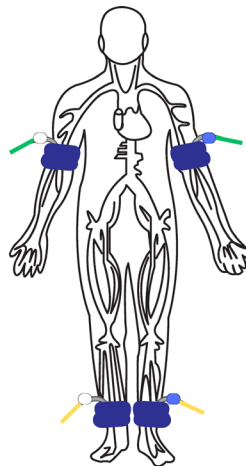

Resting Portion

Brachial Pressure

1. Begin with the right brachial. Place the Doppler probe at a 45 degree angle to the skin over the radial or brachial artery. Use plenty of gel and slowly move the probe laterally until the best signal is obtained.
2. Press and hold **Inflate** on the Cuff-Link Remote (shown above) and inflate the cuff until you no longer hear the signal - continue for an additional 10-20 mmHg.
3. Release **Inflate** and the cuff will automatically deflate at the suggested rate of 2mmHg/second.
4. When you hear the Doppler signal return, pressing **Pressure** will be store the pressure value in the exam.

Ankle Pressures

1. Press **Next** on the remote and the system will move to the Dorsalis Pedis (DP) site. Find the arterial signal using the Doppler probe on the dorsalis pedis artery on top of the foot. Obtain the arterial pressure in the same manner you did on the arm. (Hold **Inflate** until occlusion, release **Inflate**, press **Pressure** on Doppler signal return)
2. Press **Next** and the system will move to the posterior tibial (PT) site. Find the Doppler signal on the posterior tibial artery. Obtain the arterial pressure. (Hold **Inflate** until occlusion, release **Inflate**, press **Pressure** on Doppler signal return)

Waveform

1. Press **Next** and the system will move to the waveform site. Press and release the button with the **Waveform** image on the top right of the remote. The cuff will inflate to 80 mmHg pressure, slowly deflate to 65 mm and then hold that while the waveform is obtained. The waveform will start to appear when the cuff has reached 65mmHg. The patient should remain as still as possible during the measurement.

Left Side

1. Repeat the above pressures and waveform sequence for the left side of the patient.

Exercise

1. Have the patient perform 50 toe raises or until pain is prevalent OR hall walking for 5 minutes or until pain is prevalent,
2. Repeat resting ABI protocol described above.

Saving/Printing

Save the report by selecting *File* → *Save* or pressing CTRL+S. Print the report by selecting *File* → *Print* or pressing CTRL+P.

Exam Helpful Hints

Cuffs

Leave cuffs on for hall walking or toe raises but disconnect tubing.

The ABI Stress Examination

Purpose & Background

The ABI Stress-Treadmill test is useful for differentiating true vascular claudication from other non-vascular pains. The stress can be produced by treadmill walking exercise (CPT 93924) or by toe/heel raises (CPT 93923).

Contraindications

- Questionable cardiac status
- Severe pulmonary disease
- Ischemic rest pain, ulceration, or ankle pressures <40mm Hg
- Non-compressible tibial arteries
- Do not perform the ABI exam on someone suspected of having acute deep venous thrombosis, and do not take an arm pressure in an arm with a shunt or dialysis graft.


Explain to the patient that they will be exercising, either walking or doing toe raises, or until pain stops them. Ask them to tell you when and where pain occurs. Remind them to report any chest pain, shortness of breath, or severe fatigue.

Opening the exam

On the computer desktop, double click the simpleABI icon. When the program opens select *File* → *New* → *New ABI Stress - Treadmill Report*. The report will open and you can enter patient information, risk factors, symptoms, ICD codes, etc.

Attaching cuffs

Wrap appropriate cuffs at each site. Attach the hoses from the Cuff-Link control unit to cuffs as shown below. The green connectors go to the arm cuffs and yellow to the ankles. White hoses go to the patient's right side, blue to the left. *NOTE* the image is reversed as if you are looking at the patient lying down

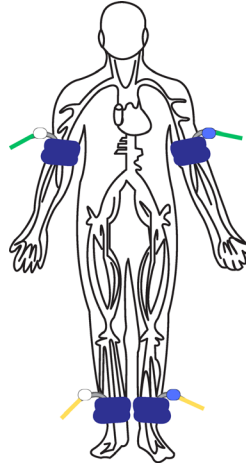

Brachial Pressure

1. Begin with the right brachial. Place the Doppler probe at a 45 degree angle to the skin over the radial or brachial artery. Use plenty of gel and slowly move the probe laterally until the best signal is obtained.
2. Press and hold **Inflate** on the Cuff-Link Remote (shown above) and inflate the cuff until you no longer hear the signal - continue for an additional 10-20 mmHg.
3. Release **Inflate** and the cuff will automatically deflate at the suggested rate of 2mmHg/second.
4. When you hear the Doppler signal return, pressing **Pressure** will store the pressure value in the exam.

Ankle Pressures

1. Press **Next** on the remote and the system will move to the Dorsalis Pedis (DP) site. Find the arterial signal using the Doppler probe on the dorsalis pedis artery on top of the foot. Obtain the arterial pressure in the same manner you did on the arm. (Hold **Inflate** until occlusion, release **Inflate**, press **Pressure** on Doppler signal return)
2. Press **Next** and the system will move to the posterior tibial (PT) site. Find the Doppler signal on the posterior tibial artery. Obtain the arterial pressure. (Hold **Inflate** until occlusion, release **Inflate**, press **Pressure** on Doppler signal return)

Waveform

1. Press **Next** and the system will move to the waveform site. Press and release the button with the **Waveform** image on the top right of the remote. The cuff will inflate to 80 mmHg pressure, slowly deflate to 65 mm and then hold that while the waveform is obtained. The waveform will start to appear when the cuff has reached 65mmHg. The patient should remain as still as possible during the measurement.

Left Side

1. Repeat the above pressures and waveform sequence for the left side of the patient.

Exercise

1. Have the patient walk on treadmill at 1-2MPH, 10% grade, for 5 minutes or until pain precludes the patient from walking further.
2. Repeat resting ABI protocol described above immediately following exercise and monitor for up to 5 more periods.

Saving/Printing

Save the report by selecting *File* → *Save* or pressing CTRL+S. Print the report by selecting *File* → *Print* or pressing CTRL+P.

Exam Helpful Hints

Cuffs

Leave cuffs on for treadmill protocol but disconnect tubing.

Chapter 6 – Detailed Description

Operation and Use

The Doppler, probes, and pressure sensors are designed to aid in diagnosis of vascular conditions including aiding in obtaining systolic pressures during an ABI examination.

Turning the unit ON/OFF

Power to the unit is controlled by the **ON/OFF** button located in the center of the Cuff-Link Control Unit. Pressing and releasing the button will cycle the unit through the power sequence. The LED in the power button will remain illuminated during operation.

Volume

The Doppler has multiple volume levels. These are controlled with the volume up and down buttons.

Probes:

D8 - 8 MHz – Vascular. simpleABI Systems come standard with an 8MHz probe designed for locating shallow lying vessels. The pen-tip sensor face aids in the location of specific vessels during examination.

D5 - 5 MHz – Vascular. An optional 5MHz probe is available for simpleABI Systems and designed for locating deeper lying vessels. The wider sensors may aid in maintaining the probe location on the vessel during examination.

SPPG - PPG – The Photoplethysmograph probe uses the absorption of infrared light by blood cells in the blood to produce an audible beep each time it detects a vascular pulse in the near surface vessels.

Chapter 7 – Tips & Troubleshooting

Obtaining Doppler Signals

CAUTION: For any examination utilizing a Doppler, it is essential that an adequate supply of gel is used to transmit the ultrasound energy from the probe to the surface of the skin. Re-apply more gel if it starts to dry out or spread so thinly that an air gap occurs between the probe and the skin. It is not necessary to cover the entire surface of the probe, only the probe face. Applying too much gel makes the unit difficult to clean and does not aid in the performance of the probe. Given the small area of the vascular probes, the strength of the Doppler signal is highly location specific.

Poor Sound Quality

Inadequate gel use-apply more gel

Probe location-search for vascular sounds as described in **Chapter 5 – Performing Exams**

Obtaining Waveforms

- Wrap the cuff snugly.
- While wrapping cuffs, do not let the patient try to help by lifting their leg - as soon as they relax their muscles the cuff will become loose.
- Placing a pillow under the patient's heels may aid the examination.
- Have the patient remain as still and quiet as possible while taking the waveforms.
- If the patient has tremors that interfere with the waveform, having them do a few dorsiflexions with their toes before taking the waveform can sometimes help.

Chapter 8 – Maintenance, Cleaning & Disposal

CAUTION: Newman Medical recommends leaving your computer on overnight once a week to allow for system updates to occur while system is not in use.

CAUTION: simpleABI components are not designed for liquid immersion. Do not soak or drop the Doppler probes in liquid.

CAUTION: The equipment is not designed for sterilization processes such as autoclaving or gamma radiation.

The equipment require very little maintenance. It is important, however, for the continued functionality of the unit and the safety of the patients to that the unit is cleaned and examined regularly as follows:

After every examination

Excess gel should be wiped off after each examination. Probe should be cleaned with a damp water or alcohol based wipe. Mild soap or detergent can be used. In particular, pay attention to any surface openings on the unit including, but not limited to, the speaker grill, the audio output, and the parting line between the front and back shell.

Practitioners should wash hands and change gloves after every exam. Please follow local and hospital guidelines for cleaning and disinfection policies.

To disinfect unit, use an appropriate disinfectant spray or wipe and follow the manufacturer's instructions.

Store unit in a clean area free from dust and debris in an indoor environment.

Periodically

Inspect the system for signs or cracks or breaks in the surface housing. If any sign of cracking or damage is evident, use of the unit should be discontinued. Please contact Newman Medical for service.

Inspect the cuffs for damage. Cuff covers may be washed by removing the bladders.

Disposal

This device and accessories must be disposed of according to local regulations after their useful lives. Alternatively, they may be returned to Newman Medical for recycling and proper disposal.

Chapter 9 – Specifications

Level of Protection against electrical shock

Type B Applied Part; Class II Equipment

Designed to meet the following standards:

IEC60601-1, IEC60601-2, IEC60601-2-37

simpleABI System

Height (inclusive) 107 cm (42 inches)
 Weight (inclusive) 5.5 kgs (12 pounds)
 Handling Temperature 10° ~ 40° C (50° ~ 104° F)
 Handling Humidity 30% ~ 75%, non-condensing
 Transport/Storage Temperature -20° ~ 50° C (-4° ~ 122° F)
 Transport/Storage Humidity 5% ~ 90%, non-condensing
 Battery Life 10 hours

Acoustic Properties

System: DigiDop Operating Mode: Continuous Wave (CW)
 Transducer Model: 5MHz Application(s): Peripheral Vascular

Acoustic Output		MI	I _{SPTA.3} (mW/cm ²)	I _{SPPA.3} (mW/cm ²)	
Global Maximum Value		0.0223	86.4	86.4	
Associated Acoustic Parameters	p _{r.3} (Mpa)	0.041			
	W _o (mW)		9.26	9.26	
	f _c (MHz)	5.61	5.61	5.61	
	Z _{sp} (cm)	1.10	1.10	1.10	
	Beam Dimensions	x-6 (cm)		0.154	0.154
		y-6 (cm)		0.540	0.540
	PD (usec)	CW		CW	
	PRF (Hz)	n/a		n/a	
	EBD	Az. (cm)		1.052	
Ele. (cm)			0.526		

System: DigiDop Operating Mode: Continuous Wave (CW)
 Transducer Model: 8MHz, narrow Application(s): Peripheral Vascular

Acoustic Output		MI	I _{SPTA.3} (mW/cm ²)	I _{SPPA.3} (mW/cm ²)	
Global Maximum Value		0.0495	555	555	
Associated Acoustic Parameters	p _{r.3} (Mpa)	0.0923			
	W _o (mW)		9.02	9.02	
	f _c (MHz)	7.84	7.84	7.84	
	Z _{sp} (cm)	0.50	0.50	0.50	
	Beam Dimensions	x-6 (cm)		0.231	0.231
		y-6 (cm)		0.121	0.121
	PD (usec)	CW		CW	
	PRF (Hz)	n/a		n/a	
	EBD	Az. (cm)		0.203	
Ele. (cm)			0.457		

Measurement Uncertainties:

Total uncertainty for power: 28.2%
 Total uncertainty for I_{SPTA}: 28.2%
 Total uncertainty for f_c: 2.0%
 Total uncertainty for MI: 14.1%

I_{SPTA.3} **derated spatial-peak temporal-average intensity** (milliwatts per square centimeter).

I_{SPPA.3} **derated spatial-peak pulse-average intensity** (watts per square centimeter). The value of IPA.3 at the position of global maximum MI (IPA.3@MI) may be reported instead of ISPPA.3 if the global maximum MI is reported.

MI	Mechanical Index. The value of MI at the position of ISPPA.3, (MI@ISPPA.3) may be reported instead of MI (global maximum value) if ISPPA.3 is $\leq 190\text{W/cm}^2$.
$p_{r,3}$	derated peak rarefactional pressure (megapascals) associated with the transmit pattern giving rise to the value reported under MI.
W_0	ultrasonic power (milliwatts). For the operating condition giving rise to ISPTA.3, W_0 is the total time-average power; for the operating condition subject to reporting under ISPPA.3, W_0 is the ultrasonic power associated with the transmit pattern giving rise to the value reported under ISPPA.3.
f_c	center frequency (MHz). For MI and ISPPA.3, f_c is the center frequency associated with the transmit pattern giving rise to the global maximum value of the respective parameter. For ISPTA.3, for combined modes involving beam types of unequal center frequency, f_c is defined as the overall range of center frequencies of the respective transmit patterns.
z_{sp}	the axial distance at which the reported parameter is measured (centimeters).
x_{-6}, y_{-6}	are respectively the in-plane (azimuthal) and out-of-plane (elevational) -6 dB dimensions in the x-y plane where z_{sp} is found (centimeters).
PD	pulse duration (microseconds) associated with the transmit pattern giving rise to the reported value of the respective parameter.
PRF	the pulse repetition frequency (Hz) associated with the transmit pattern giving rise to the reported value of the respective parameter.
EBD	the entrance beam dimensions for the azimuthal and elevational planes (centimeters).
EDS	the entrance dimensions of the scan for the azimuthal and elevational planes (centimeters).

The reporting values for ultrasonic power, W_0 , and non-derated spatial average temporal average ISATA required by paragraph 2.1.2 of the FDA Guidance [3] as well as the derated spatial-peak temporal-average intensity, ISPTA.3, provided for reference only, are calculated for all probes as illustrated in the sample calculations below.

For Non-Auto scanning modes reporting parameters are calculated as:

$$W_0 = I_{SPTA,0} * PF$$

$$I_{SATA,0} = W_0 / (\text{entrance beam area})$$

$$I_{SPTA,3} = I_{SPTA,0} * e^{-0.069 f_c z}$$

Where $I_{SPTA,0}$, is the non-derated spatial-peak temporal-average intensity, $I_{SATA,0}$ is the nonderated spatial-average temporal-average intensity at the transducer face and $I_{SPTA,3}$, is the derated spatial-peak temporal-average intensity, f_c , the waveform center frequency, z , the axial distance between the probe and hydrophone, PF, the power factor which is calculated by integrating the normalized cross axis and raster scan data selecting the largest PF value, which is an “effective area” used to calculate W_0 , the ultrasonic power.

Chapter 10 – Electromagnetic Compatibility

All medical equipment may produce electromagnetic interference or be susceptible to electromagnetic interference. The following are guidance and manufacturer’s declarations regarding EMC for SimpleABI.

- simpleABI Systems need special precautions regarding EMC and needs to be installed and put into service according to the EMC information provided in the following pages.
- **Warning:** This equipment is intended for use by healthcare professionals only. As with all electrical medical equipment, this equipment may cause radio interference or may disrupt the operation of nearby equipment. It may be necessary to take mitigation measures such as re-orienting or relocating the SimpleABI system or shielding the location.
- Portable and Mobile RF communications equipment can affect the performance of SimpleABI. Please use the guidelines and recommendations specified in Tables 15.3.1 and 15.3.2.
- Other Medical Equipment or Systems can produce electromagnetic emissions and therefore can interfere with the functionality of SimpleABI. Care should be used when operating SimpleABI adjacent to or stacked with other equipment. If adjacent or stacked use is necessary, SimpleABI should initially be observed to verify normal operation in the configuration in which it will be used.
- The electrical cables, external power supplies and accessories listed or referenced in this manual have been shown to comply with the test requirements listed in the following tables. Care should be taken to use only manufacturer-recommended cables, power supplies and electrical accessories with SimpleABI. If a third-party supplier offers cables, external power supplies and electrical accessories for use with SimpleABI and they are not listed or referenced in this manual, it is the responsibility of that third-party supplier to determine compliance with the standards and tests in the following tables.
- The use of electrical cables and accessories other than those specified in this manual or referenced documents may result in increased electromagnetic emissions from SimpleABI or decreased electromagnetic immunity of SimpleABI.

Table for Electromagnetic Emissions


Guidance and Manufacturer’s Declaration – Electromagnetic Emissions		
The simpleABI System is intended for use in the electromagnetic environment specified below. The customer or the user of the device should assure that it is used in such an environment.		
Emissions test	Compliance	Electromagnetic environment - guidance
RF Emissions - CISPR 11 (Radiated & Conducted)	Group 1	The simpleABI System uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF Emissions - CISPR 11 (Radiated & Conducted)	Class B	The simpleABI System is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.

Table for Electromagnetic Immunity

Guidance and Manufacturer’s Declaration – Electromagnetic Immunity
The simpleABI System is intended for use in the electromagnetic environment specified below. The customer or the end user should assure it is used in such an environment.

Immunity Test	EN/IEC 60601 Test Level	Compliance Level	Intended Electromagnetic Environment
Electromagnetic Discharge (ESD) EN/IEC 61000-4-2	± 6kV contact ± 8kV air	± 6kV contact ± 8kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.
Electrical fast transient/burst EN/IEC 61000-4-4	± 2kV for power supply lines ± 1kV for input/output lines	± 2kV for power supply lines ± 1kV for input/output lines	Mains power quality should be that of a typical commercial or hospital environment.
Power frequency (50/60Hz) magnetic field EN/IEC 61000-4-8	3A/m	3A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.

Guidance and Manufacturer’s Declaration – Electromagnetic Immunity (continued)

Immunity Test	EN/IEC Test Level	60601 Compliance Level	Intended Electromagnetic Environment
Conducted RF EN/IEC 61000-4-6	3Vrms 150kHz to 80MHz	3Vrms 150kHz to 80MHz	<p>Portable and mobile RF communications equipment should be used no closer to any part of SimpleABI, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.</p> <p>Recommended separation distance</p> <p>$d = 1.2\sqrt{P}$ 80MHz to 800 MHz</p> <p>$d = 2.3\sqrt{P}$ 800MHz to 2.5GHz</p> <p>where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended minimum separation distance in meters (m).</p> <p>Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey^a, should be less than the compliance level in each frequency range.^b</p> <p>Interference may occur in the vicinity of equipment marked with the following symbol:</p>
Radiated RF EN/IEC 61000-4-3	3V/m 80MHz to 2.5GHz	3V/m 80MHz to 2.5GHz	

NOTE 1: At 80MHz and 800MHz, the higher frequency range applies.

NOTE 2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from objects, structures and people.

^a Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the SimpleABI is used exceeds the applicable RF compliance level above, the SimpleABI should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the SimpleABI.

^b Over the frequency range 150kHz to 80MHz, field strengths should be less than 3V/m.

Recommended separation distances between portable and mobile RF communications equipment and the SimpleABI.

SimpleABI unit is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of SimpleABI can help prevent electromagnetic interference by maintaining a minimum distance between the portable and mobile RF communications equipment (transmitters) and SimpleABI as recommended below, according to the maximum output power of the communications equipment.

Rated maximum output power of transmitter in watts (W)	Separation distance according to frequency of transmitter in meters (m)		
	150kHz to 80MHz <i>d = 1.2√P</i>	80MHz to 800MHz <i>d = 1.2√P</i>	800MHz to 2.5GHz <i>d = 2.3√P</i>
0.01	.12	.12	.23
0.1	.38	.38	.73
1.0	1.2	1.2	2.3
10	3.8	3.8	7.3
100	12	12	23

For transmitters rated at a maximum output power not listed above, the recommended separation distance (d) in meters (m) can be estimated using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

NOTE 1: At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

NOTE 2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

Chapter 11 – Warranty, Service, & Support

The simpleABI System and components are guaranteed to be free from defects in material and workmanship for 2 years from the original sale of the device. This guarantee includes all parts and labor required to repair or replace the unit, including shipping the unit back to the customer. Customer is responsible for the adequate packaging and return of the unit for servicing. Products will be repaired or replaced in a reasonable amount of time, to be determined by service personnel.

The manufacturer and distributor of a simpleABI System assume neither responsibility nor liability for incidental or consequential damages arising from the purchase of this product.

The manufacturer and distributor of simpleABI Systems are not responsible for damages occurring from misuse or neglectful handling of the device. Any abuse, neglect, or alteration of the equipment, including dismantling of the unit (other than by trained service personnel), from its original specifications nullify all stated and implied warranties.

To return a unit for servicing:

1. Call customer service for a return authorization.
2. Clean the product prior to packing and shipping.
3. Adequately package and return the unit to:

Newman Medical
Attn: Service
5350 Vivian Street, Unit C
Arvada, CO 80002
800-267-5549