

## Cuff Cleaning and Disinfecting

Use one or more of the following methods and allow to air dry:

- Wipe with mild detergent and water solution (1:9 solution). Rinse.
- Wipe with Enzol per manufacturer's instructions. Rinse.
- Wipe with .5% bleach and water solution. Rinse.
- Wipe with 70% isopropyl alcohol.
- Launder with mild detergent in warm water, normal wash cycle. Remove bladder first. Cuff is compatible with 5 wash cycles.

## Low-Level Disinfection

Prepare Enzol enzymatic detergent according to the manufacturer's instructions. Spray detergent solution liberally onto cuff and use a sterile brush to agitate the detergent solution over entire cuff surface for five minutes. Rinse continuously with distilled water for five minutes. To disinfect, first follow the cleaning steps above, then spray cuff with 10% bleach solution until saturated, agitate with a sterile brush over entire cuff surface for five minutes. Rinse continuously with distilled water for five minutes. Wipe off excess water with sterile cloth and allow cuff to air dry.

**CAUTION:** Do not iron cuff.


**CAUTION:** Do not heat or steam sterilize cuff.

## Manometer Quality Control


A serial number and lot number are automatically assigned to every aneroid during manufacturing, ensuring every item is "controlled."

The serial number can be located on the faceplate of each aneroid (Figure 4).

The lot number is located on the box end label (Figure 5).

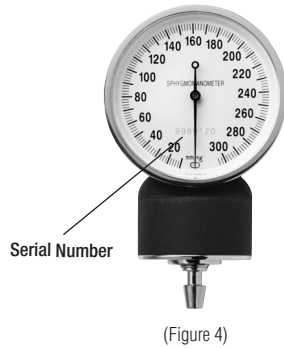

(Figure 4)

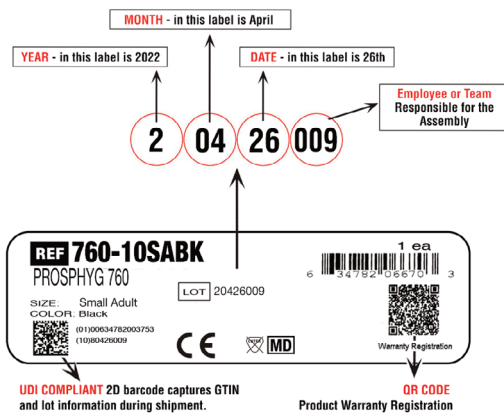

## Standards


ANSI/AAMI/ISO 81060-1:2007 • EN/ISO 81060-1:2012

## Disposal

When your sphygmomanometer or any of its parts have reached their end of life, please be sure to dispose of them in accordance with all regional and national environmental regulations. Devices that have become contaminated should be disposed of in accordance with all local ordinances and regulations.

# Prosplyg™ Aneroids

## Instructions for Use

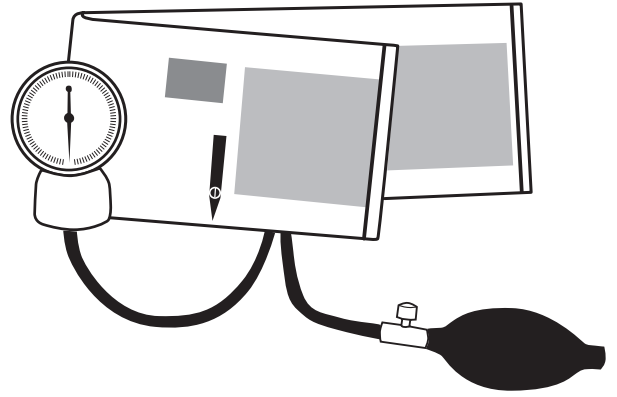

## Warranty

ADC® warrants its products against defects in materials and workmanship under normal use and service as follows:

- Warranty service extends to the original retail purchaser only and commences with the date of delivery.
- See end panel label for package contents and to determine warranty duration.

### Warranty duration is as follows:

Series	Manometer	Inflation System
760, 768, 769	20 Years	3 Years
780, 785, 790, 770, 775	10 Years	1 Year

**What Is Covered:** Replacement of parts and labor.

**What Is Not Covered:** Transportation charges. Damages caused by abuse, misuse, accident, or negligence. Incidental, special, or consequential damages. Some states do not allow the exclusion or limitation of incidental, special, or consequential damages, so this limitation may not apply to you.

**Implied Warranty:** Any implied warranty shall be limited in duration to the terms of this warranty and in no case beyond the original selling price (except where prohibited by law). This warranty gives you specific legal rights and you may have other rights which vary from state to state.

**To Obtain Warranty Service:** Send item(s) postage paid to: ADC, Attn: Repair Dept., 55 Commerce Dr., Hauppauge, NY 11788. Please include your name and address, phone no., proof of purchase, and a brief note explaining the problem.

## For Australian Consumers

Our goods come with guarantees that cannot be excluded under the Australian Consumer Law. You are entitled to a replacement or refund for a major failure and compensation for any other reasonably foreseeable loss or damage. You are also entitled to have the goods repaired or replaced if the goods fail to be of acceptable quality and the failure does not amount to a major failure.

## For our European Customers

On request, send to ADC by e-mail ([info@adctoday.com](mailto:info@adctoday.com)), we can send to you this manual on paper form within 7 calendar days at no additional cost to the user.

Our website, <https://www.adctoday.com>, where these instructions for use are available fulfills the requirements of personal data protection, according to Directive 95/46/EC and GDPR on the protection of individuals with regard to the processing of personal data and on the free movement of such data.

Any serious incident that has occurred in relation to this medical device should be reported to ADC and the competent authority of the Member State in which the user and/or patient is established.

To register your product, visit us at [www.adctoday.com/support/warranty-registration](http://www.adctoday.com/support/warranty-registration)

FOR QUESTIONS, COMMENTS, OR SUGGESTIONS CALL TOLL FREE:  
1-800-ADC-2670 or visit [www.adctoday.com/feedback](http://www.adctoday.com/feedback)

ADC  
55 Commerce Drive  
Hauppauge, NY 11788  
U.S.A.



Inspected, assembled  
and packaged in the U.S.A.

tel: 631-273-9600  
1-800-232-2670  
fax: 631-273-9659

[www.adctoday.com](http://www.adctoday.com)  
email: [info@adctoday.com](mailto:info@adctoday.com)

SC Cattus SRL  
Str. Baneasa Nr. 10 C  
Târgu-Mures, Jud. Mures  
România, EU



IB p/n 9360N-00 rev 17 (02/07/2023)

Printed in the U.S.A.

Thank you for choosing an ADC® Prosplyg™ Aneroid sphygmomanometer.

### Device Description and Intended Use

An ADC® aneroid sphygmomanometer is used by professional healthcare providers and individuals trained in the auscultatory blood pressure technique to determine systolic and diastolic blood pressure in humans.

### Contraindications

Aneroid sphygmomanometers are contraindicated for neonate use. Do not use with neonatal cuffs or neonate patients. Review the size chart (below) for proper limb range.

#### 780-790 Series Size Chart

Cuff	Size	Limb Range Inches	CM
Sm. Adult	10SA	6.3 to 9.8	16 to 25
Adult	11A	9 to 13.3	23 to 34
Lg. Adult	12X	11.8 to 15.7	30 to 40

#### Adcuff Series Size Chart

Cuff	Size	Limb Range Inches	CM
Infant	7I	3.5 to 5.5	9 to 14
Child	9C	5.1 to 7.6	13 to 19.5
Sm. Adult	10SA	7.4 to 10.6	19 to 27
Adult	11A	9 to 15.7	23 to 40
Lg. Adult	12X	13.3 to 19.6	34 to 50
Thigh	13T	15.7 to 25.9	40 to 66

### Symbol Definitions

The following symbols are associated with your ADC sphygmomanometer.

Symbol	Definition
	Important Caution
	Not made with natural rubber latex
	Phthalate free
	Consult instructions for use
	Meets essential requirements of European Medical Device Directive 93/42/EEC
	Authorized Representative in the European Community/European Union
	Manufacturer
	Temperature limit

Symbol	Definition
	Circumference size
	Humidity limitation
	Date of manufacture
	Batch Code
	Medical Device
	Unique device identifier
	Non-sterile
	Do not use if package is damaged
	Importer
	Distributor
	Catalog Number

### General Warnings

**A warning statement in this manual identifies a condition or practice which, if not corrected or discontinued immediately could lead to patient injury, illness, or death.**

**WARNING:** Do not allow a blood pressure cuff to remain on patient for more than 10 minutes when inflated above 10 mmHg. This may cause patient distress, disturb blood circulation, and contribute to the injury of peripheral nerves.

**WARNING:** If luer lock connectors are used in the construction of tubing, there is a possibility that they might be inadvertently connected to intra-vascular fluid systems, allowing air to be pumped into a blood vessel. Immediately consult a physician if this occurs.

**WARNING:** Safety and effectiveness with neonate cuff sizes 1 through 5 is not established.

**WARNING:** If this equipment is modified, appropriate inspection and testing must be conducted to ensure its continued safe use.

**WARNING:** Do not apply cuff to delicate or damaged skin. Check cuff site frequently for irritation.

**WARNING:** Only use the cuff when the range markings indicated on the cuff show that the proper cuff size is selected, otherwise erroneous readings may result.

**WARNING:** Allow space between patient and cuff. Two fingers should fit in this space if the cuff is correctly positioned.

**WARNING:** Do not apply cuff to limbs used for IV infusion.

**WARNING:** Patient should remain still during measurement to avoid erroneous readings.

**WARNING:** When using with an infant or child cuff, extra care must be taken to prevent over-inflation. With smaller cuffs (infant or child) the cuff can inflate to over 300mmHg with just two full compressions of the bulb. To prevent discomfort or injury to the patient and damage to the instrument, bulb should only be partially squeezed, so that each "stroke" inflates the cuff in 40mmHg to 60mmHg increments until inflated to the desired level.

**CAUTION:** To obtain the greatest accuracy from your blood pressure instrument, it is recommended that the instrument be used within a temperature range of 50°F to 104°F (10°C to 40°C), with a relative humidity range of 15%-85% (non-condensing).

**CAUTION:** Extreme altitudes may affect blood pressure readings. Your device has been designed for normal environmental conditions.

### Operation of Pocket Aneroids


This booklet contains operating and maintenance information for pocket aneroid sphygmomanometers. Please read and retain.

Your pocket aneroid sphygmomanometer consists of an aneroid manometer (gauge), complete inflation system, (latex-free inflation bladder, squeeze bulb, and the valve), a zippered carrying case, and operating instructions.

Most models are preassembled and ready for use.

In units requiring assembly, the bulb and valve should connect to the tube closest to the Index Line. The gauge connects to the remaining tube.

Apply a small amount of alcohol or soapy water to tubing if needed.

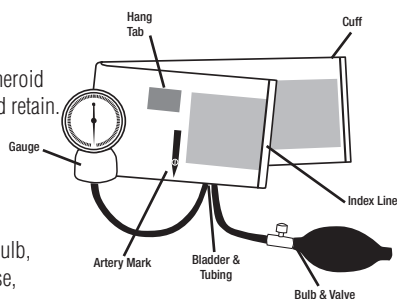


### Measurement Procedure

#### Patient Position

The patient should sit or lie comfortably. The arm should be fully supported on a flat surface at heart level. (If the arm's position varies, or is not level with the heart, measurement values obtained will not be consistent with the patient's true blood pressure.) When seated, the patient should have their back and arm supported, and their legs should not be crossed. The patient should relax prior to measurement comfortably for five minutes and should refrain from talking or moving during measurement. Observer should view manometer in a direct line to avoid "parallax error."

#### Apply the Cuff


Nylon cuffs are specially designed to promote the precisely accurate determination of blood pressure. Index and range markings ensure use of the correct cuff size. The artery mark indicates proper cuff positioning.

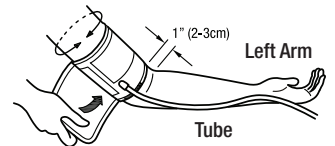

(Figure 1)

Place the cuff over the bare upper arm with the artery mark positioned directly over the brachial artery. The bottom edge of the cuff should be positioned approximately one inch (2-3cm) above the antecubital fold. Wrap the end of the cuff not containing the bladder around the arm snugly and smoothly and engage adhesive strips (Figure 1).

**NOTE:** If the unit is equipped with a calibrated nylon cuff, featuring Index and Range markings, a correct fit may be verified by checking that the Index Line falls between the two Range Lines. (Figure 2).

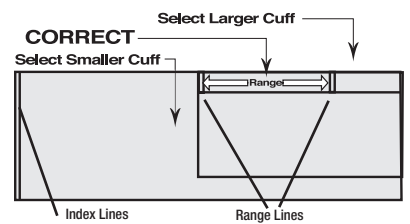

(Figure 2)

#### Inflate the Cuff

Close the valve by turning thumbscrew clockwise.

Palpate the radial artery while inflating the cuff. Be sure to inflate cuff quickly by squeezing bulb rapidly.

Inflate cuff 20-30 mmHg above the point at which the radial pulse disappears.

**NOTE:** Cuff pressure range is 0 mmHg to 300 mmHg.

#### Position the Stethoscope

Position the chestpiece in the antecubital space below the cuff, distal to the brachium. Do not place chestpiece underneath the cuff, as this impedes accurate measurement. Use the bell side of a combination stethoscope for clearest detection of the low pitched Korotkoff (pulse) sounds.

#### Deflate the Cuff

Open the valve to deflate the cuff gradually at a rate of 2-3 mmHg per second.

#### Measurement

Record the onset of Korotkoff sounds as the systolic pressure, and the disappearance of these sounds as diastolic pressure. (Some healthcare professionals recommend recording diastolic 1 and diastolic 2. Diastolic one occurs at phase 4.)

**NOTE:** It is recommended that K4 be used in children aged 3 to 12, and K5 should be used for pregnant patients unless sounds are audible with the cuff deflated, in which case K4 should be used. K5 should be used for all other adult patients.

After measurement is completed, open valve fully to release any remaining air in the cuff. Remove cuff.

### Care and Maintenance

#### STORAGE

**Pocket Gauge:** After measurement, fully exhaust cuff then wrap cuff around gauge and bulb and store in zippered carrying case.


**NOTE:** This product will maintain the safety and performance characteristics specified at temperatures ranging from 50°F to 104°F (10°C to 40°C) at a relative humidity level of 15% to 85%.

This device can be safely stored at temperatures ranging from -4°F to 131°F (-20°C to 55°C) with a relative humidity of 85% or below.

**Manometer:** Your pocket aneroid gauge requires minimal care and maintenance.

The manometer may be cleaned with a soft cloth but should not be dismantled under any circumstances.

Should the indicator needle of the manometer rest outside the oval calibration mark (Figure 3), then the manometer must be re-calibrated to within ±3 mmHg when compared to a reference device that has been certified to national or international measurement standards. A manometer whose indicator needle is resting outside of this mark is NOT acceptable for use.



**NOTE:** Store gauge with valve in full exhaust position. (Figure 3)

In the event that the gauge is ever in need of calibration, simply return for service. Damaged or broken parts will be replaced as needed at a minimal charge. Refer to the warranty for specific details of warranty coverage.

The manufacturer recommends a calibration check every 2 years.